
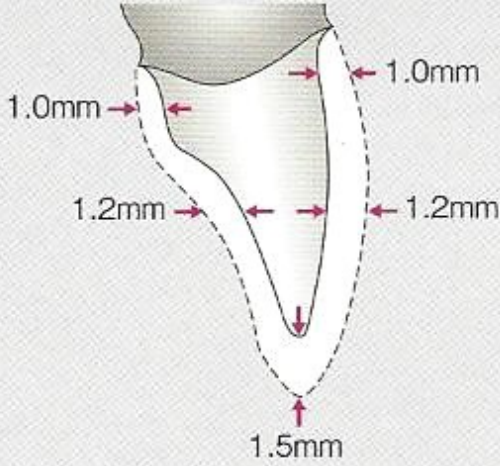
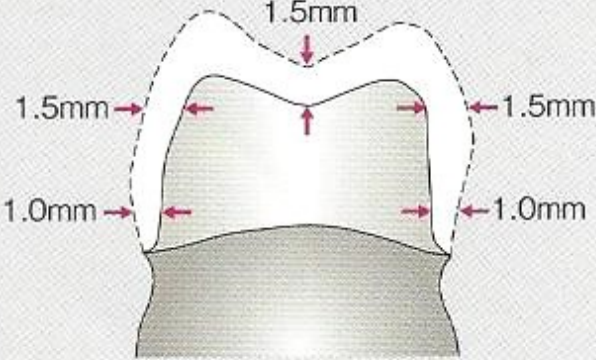
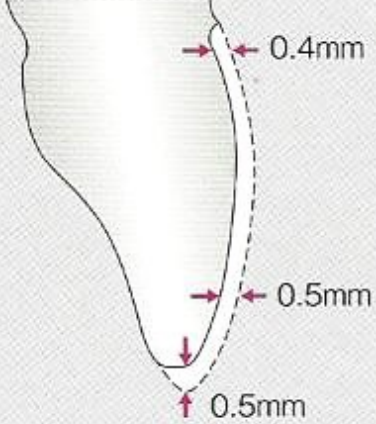
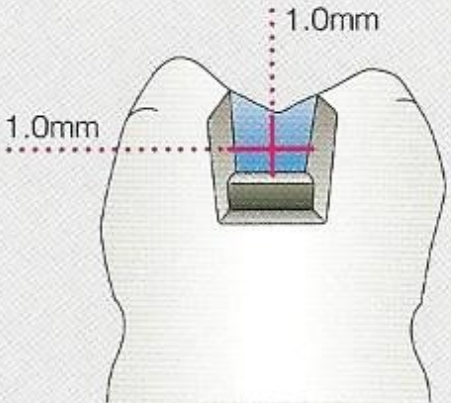


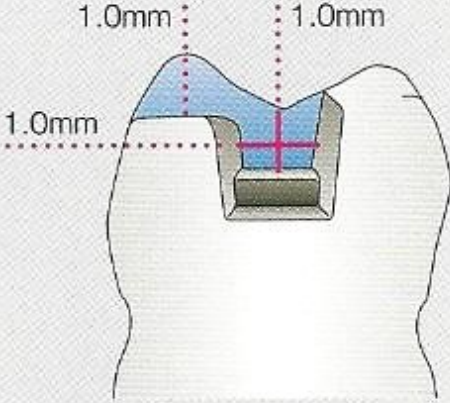

Mountain Dental Lab, Inc.

1401 Smokey Park Hwy | Candler, NC | 28715 | 828.665.2257

Minimum thickness

Anterior crown	Posterior crown	
 <p>Diagram illustrating the minimum thickness requirements for an anterior crown. The thickness is specified at various points: 1.0mm at the incisal edge, 1.2mm at the incisal angle, 1.5mm at the cervical margin, and 1.0mm at the lingual margin.</p>	 <p>Diagram illustrating the minimum thickness requirements for a posterior crown. The thickness is specified at various points: 1.5mm at the incisal edge, 1.5mm at the incisal angle, 1.0mm at the cervical margin, and 1.0mm at the lingual margin.</p>	
Veneer	Inlay	Onlay
 <p>Diagram illustrating the minimum thickness requirements for a veneer. The thickness is specified at various points: 0.4mm at the incisal edge, 0.5mm at the incisal angle, and 0.5mm at the cervical margin.</p>	 <p>Diagram illustrating the minimum thickness requirements for an inlay. The thickness is specified as 1.0mm at the incisal edge and 1.0mm at the cervical margin.</p>	 <p>Diagram illustrating the minimum thickness requirements for an onlay. The thickness is specified as 1.0mm at the incisal edge and 1.0mm at the cervical margin.</p>